


The following photos are actual photos of the laser settings for the equipment that will be used during the clinical exam.

SLT Settings



YAG Settings

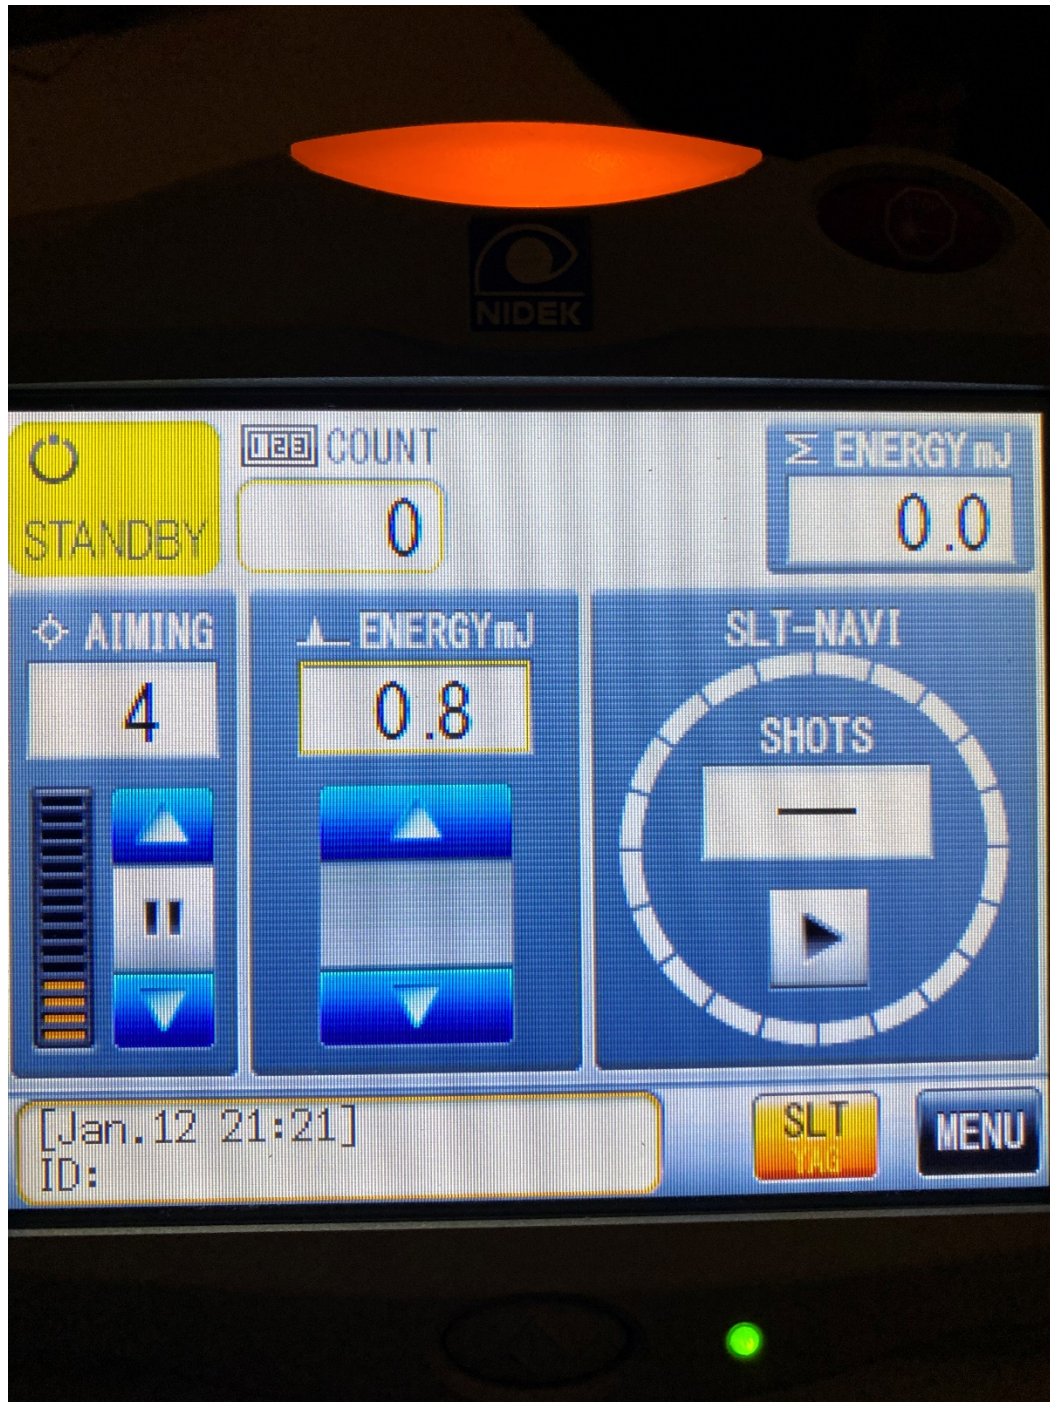